
Inventor: William Rogers - Application #10/627,286 Phone: 210-860-3655 - Email: BehaviorResearch@aol.com

FIGURE (1) Simulated view, example inside **EBA** "The Thinking Cap" which sits elevated over patient's head.

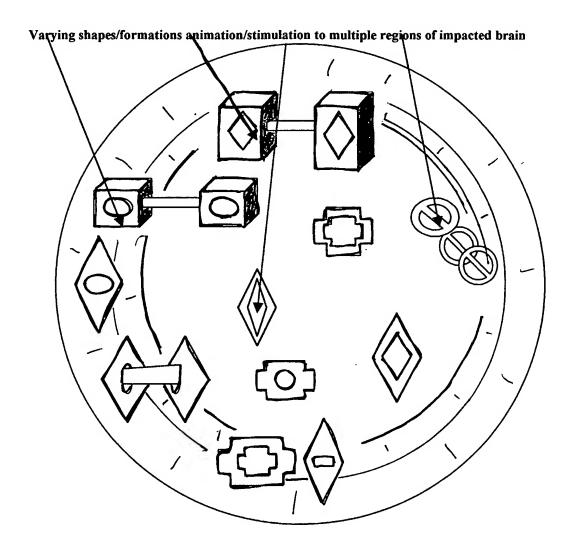


Inventor: William Rogers - Application # 10/627,286 Phone: 210-860-3655 - Email: BehaviorResearch@aol.com

FIGURE (2) Is the adjustable, pliable, conductive plate situated inside "Thinking Cap" top and around front/back, L-side/R-side, normally one half to three quarters of an inch above the contacts/coils all-round the skull area.


Inventor" William Rogers - Application # 10/627, 286 Phone: 210-860-3655 - Email: BehaviorResearch@aol.com

FIGURE 3 - Are the 7 to 10 pliable/padded "prongs", moveable/adjustable, by which "The Thinking Cap" is fixated and situated on the patient's head previous to treatment.

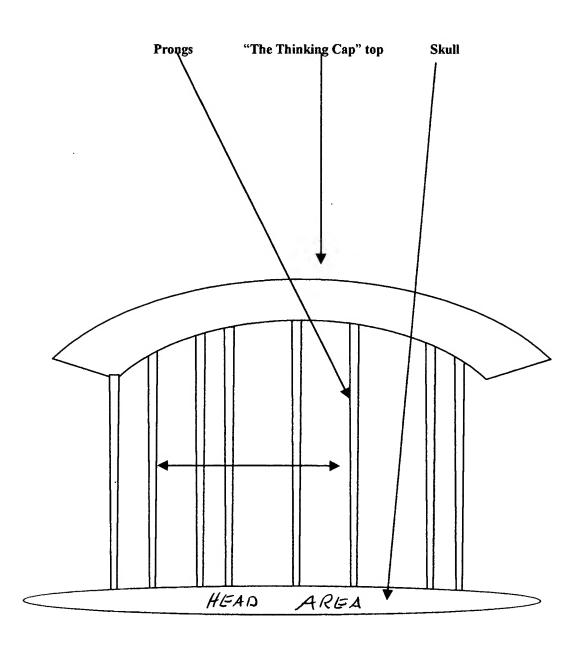


Inventor: William Rogers - Application #10/627,286 Phone: 210-408-1804 - Email: BehaviorResearch@aol.com

IGURE (4) Is illustration of phenomenon of directional specificity > a single coil at the vertex can stimulate tissue according to the direction. The image shows basic current flow in singularity with induced currents from one round coil hand-held above patient's head.).

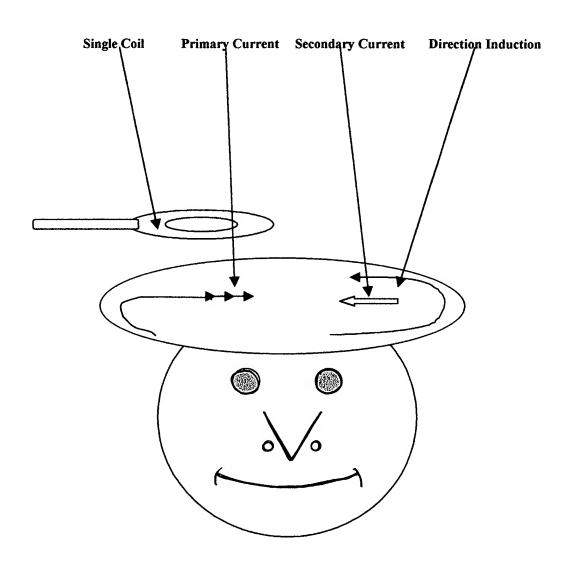


"Electromagnetic Brain Animation"
Inventor: William Rogers - Application #10/627,286
Phone: 210-860-3655 - Email: BehaviorResearch@aol.com

FIGURE (5) Shows multiple examples EBA coils in varying configurations.

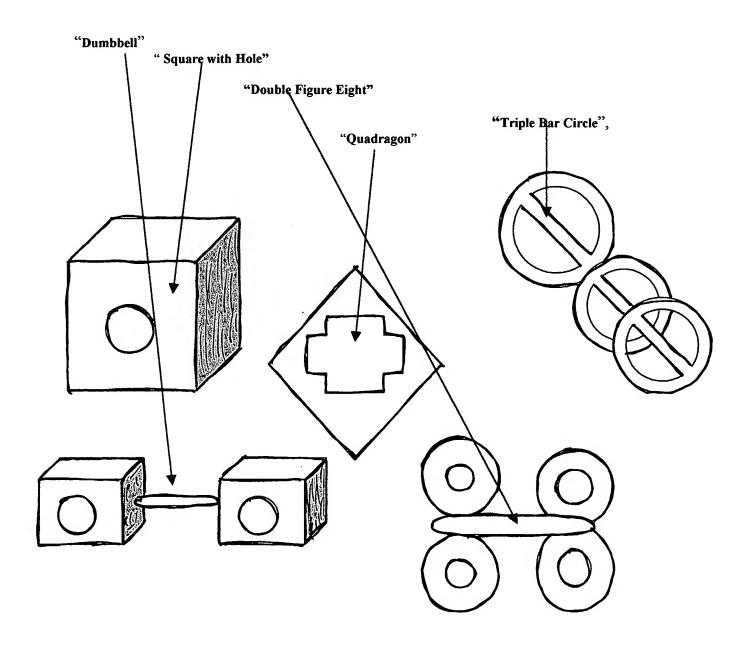


Inventor: William Rogers - Application #10/627, 286 Phone: 210-860-3655 - Email: BehaviorResearch@aol.com

FIGURE 6 Summarizes the basic chain of events pertaining to general non-invasive processes. The induced E is strongest near the coil and typically stimulates a cortical area of a few centimeters in diameter.

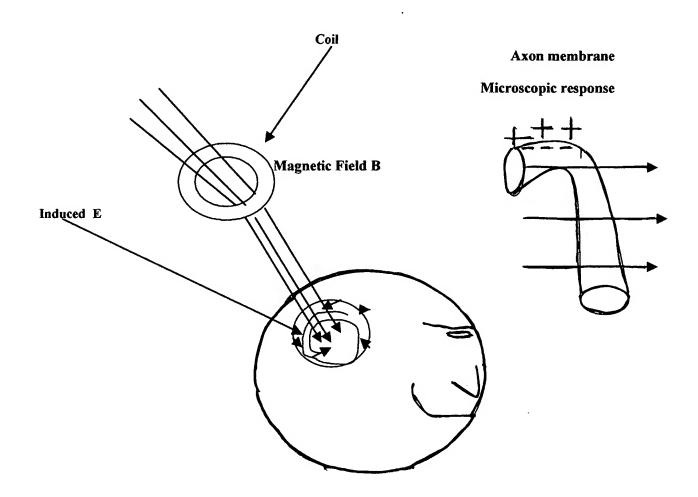

Inventor: William Rogers - Application #10/627,286 Phone: 210-860-3655 - Email: BehaviorResearch@aol.com


FIGURE (7) Shows differentiation between early childhood development habituation and highest plasticity relating to critical time for peak window of opportunity.

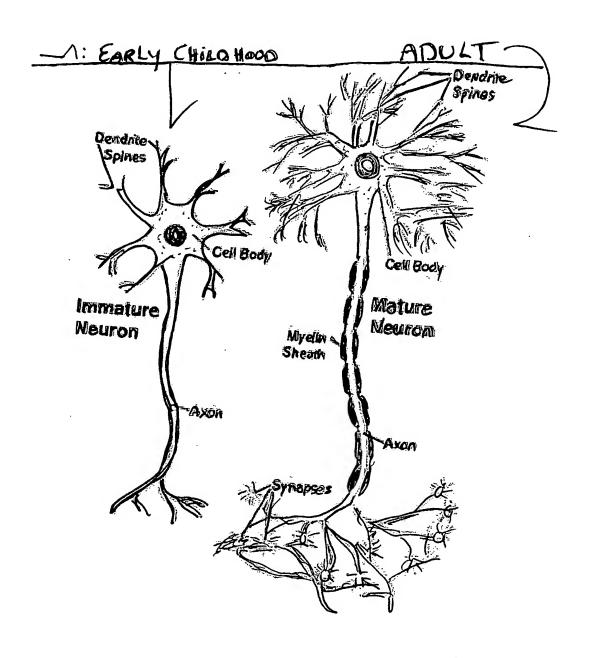

Inventor: William Rogers - Application #10/627,286 Phone: 210-860-3655 - Email: BehaviorResearch@aol.com


FIGURE (8) A schematic illustration of activation mechanisms and axon membrane polarization in a transverse field is shown for varying external applications of electric field patterns.

Axon membrane polarization sketched for different externally applied electric field patterns (arrows).:

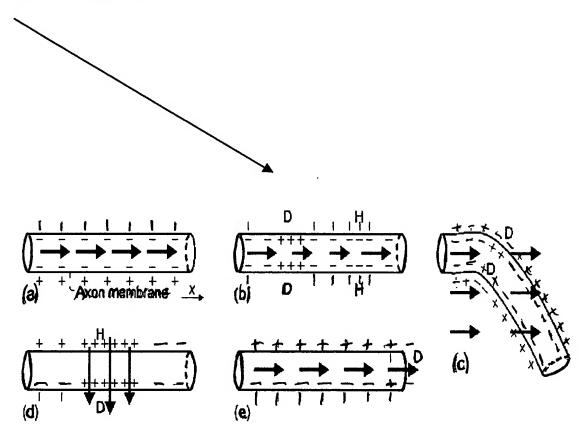


Inventor - William Rogers - Application #10/627, 286 Phone: 210-860-3655 - Email: BehaviorResearch@aol.com

FIGURE 9- Refers use of multiple independently controlled animating coils allowing heretoforeunattainable animation/stimulation data as result of varying formation, numbers, placement and specificity of coils

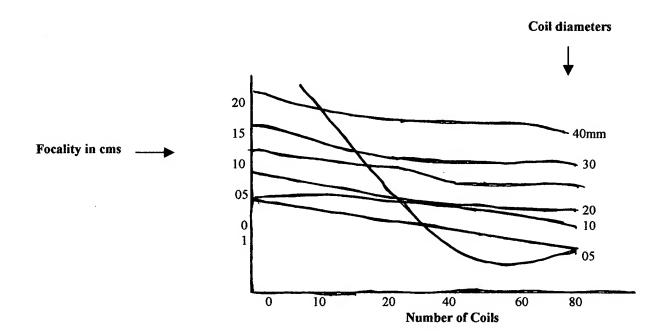

Inventor: William Rogers - Application #10/627,286 Phone: 210-860-3655 - Email: BehaviorResearch@aol.com

FIGURE (10) Outer "mechanistic" view of "Thinking Cap", adjustable prongs, adjustable chin stability assistance, and other so-named parts of instrumentation

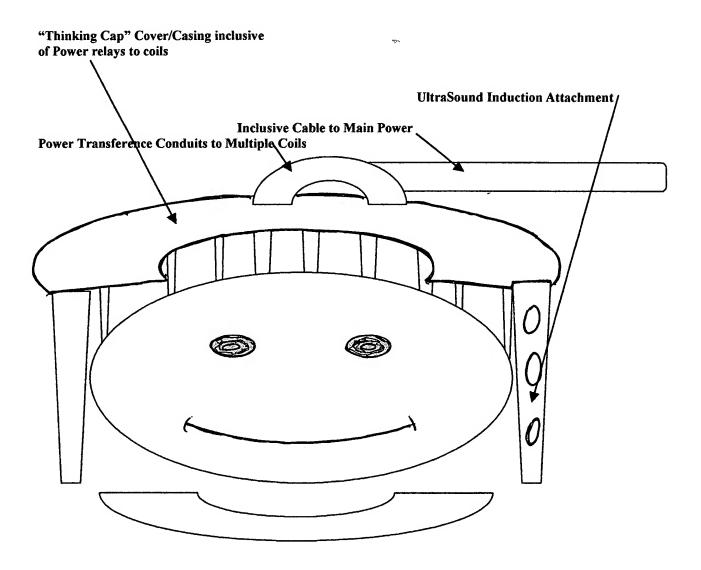

Inventor: William Rogers - Application # 10/627,286 Phone: 210-860-3655 - Email: BehaviorResearch@aol.com

FIGURE 11- Shows the initial treatment modality relating to EBA/US whereas ultrasonic waves vibrating at frequencies greater than 20,000 cycles per second are integrated through the human/patient's skull and into an excitation focal area.

